

FIG. 1

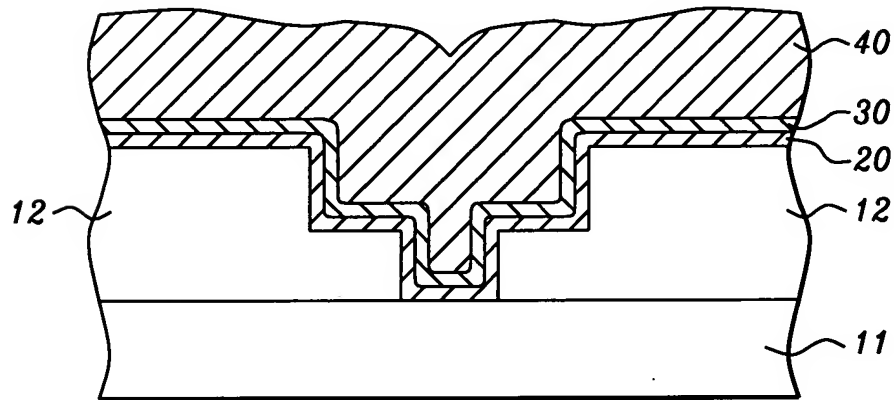


FIG. 2

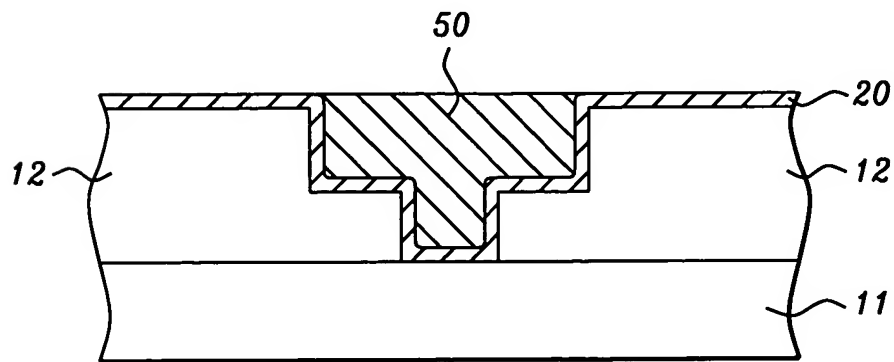
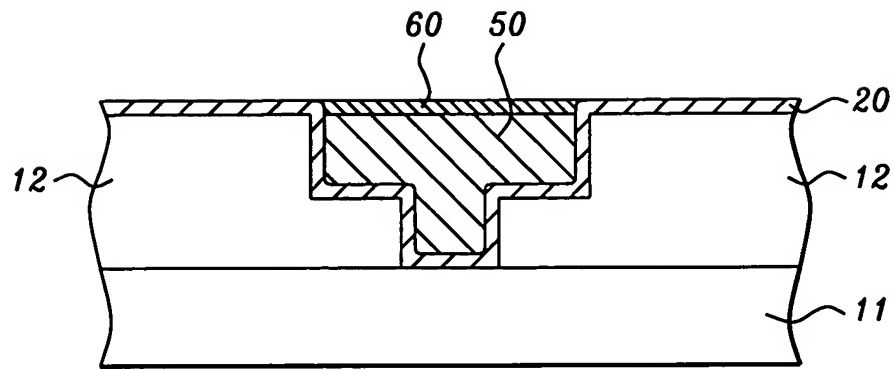
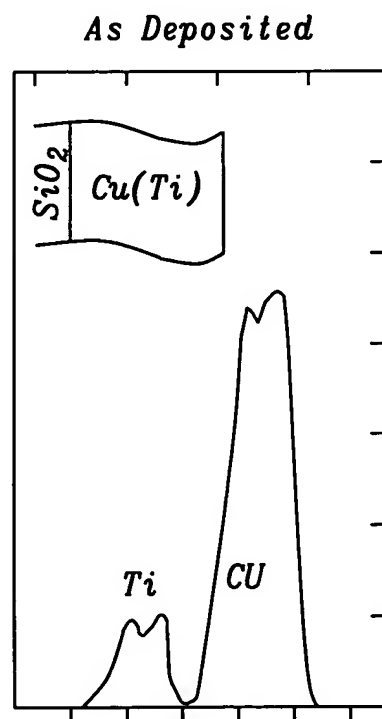


FIG. 3

*FIG. 4**FIG. 5*

400°C 30 min in NH_3



FIG. 6

550°C 30 min in NH_3

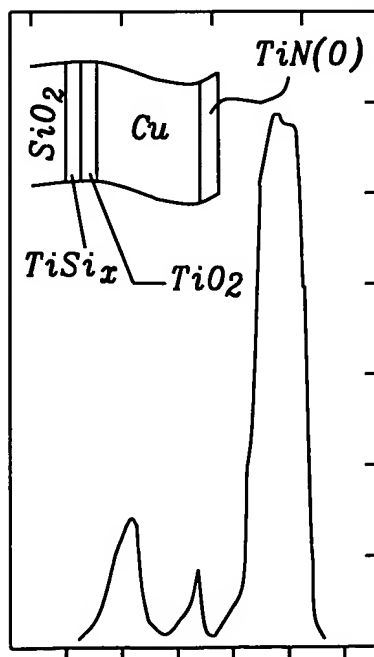


FIG. 7